

FIG. 1A

1042290 95646860

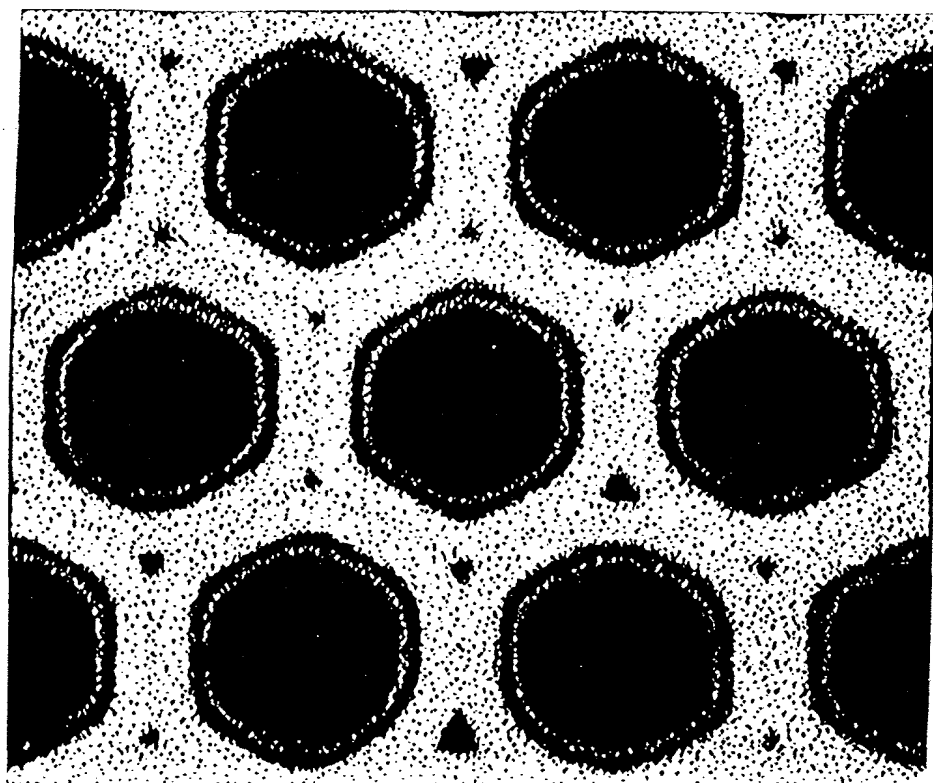


FIG. 1B

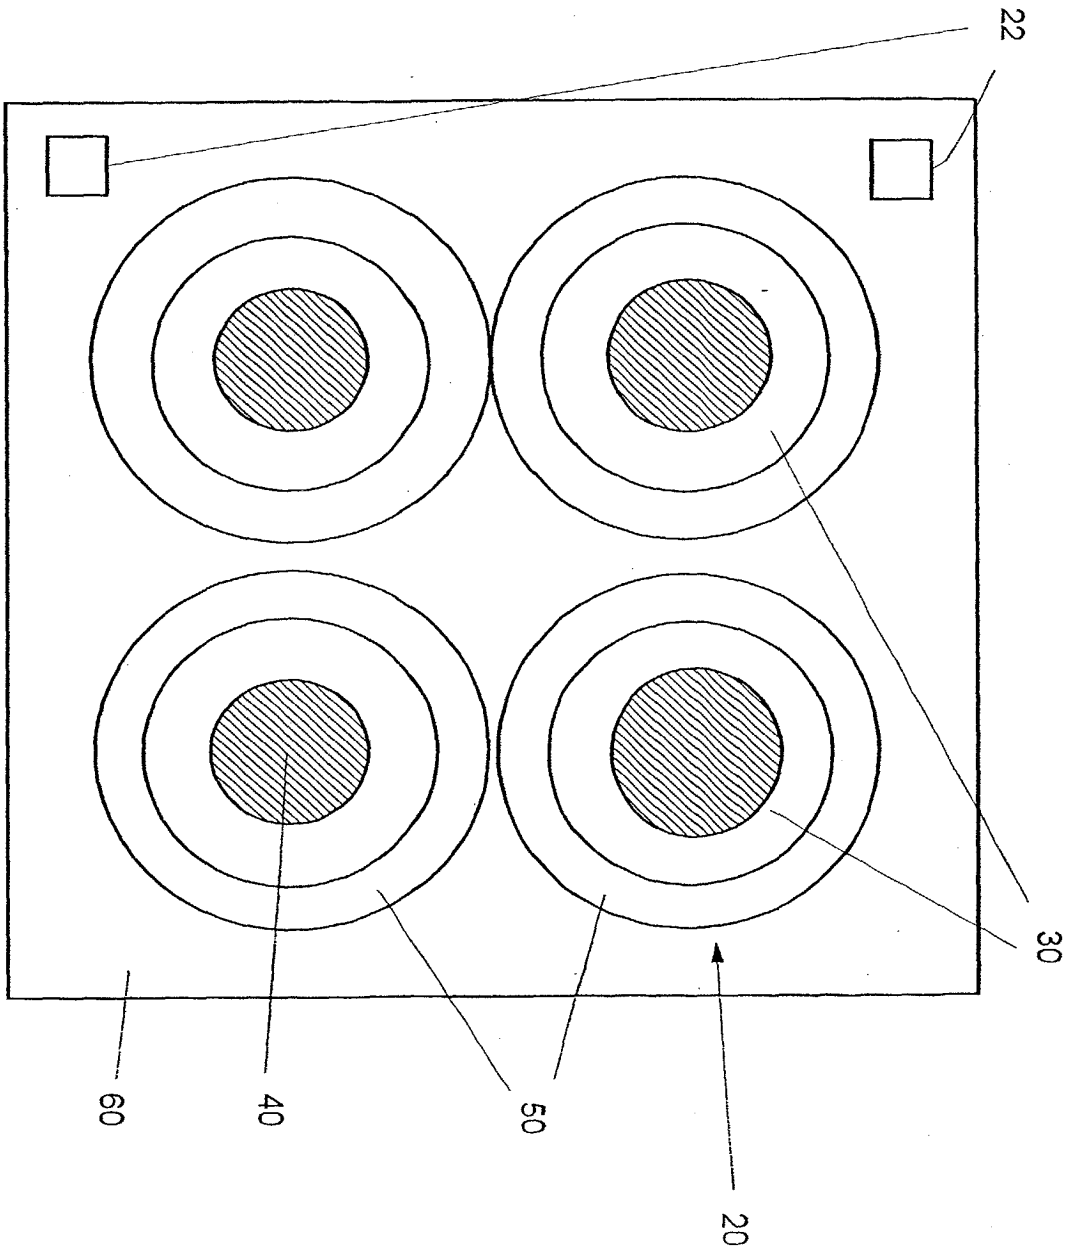


FIG. 2

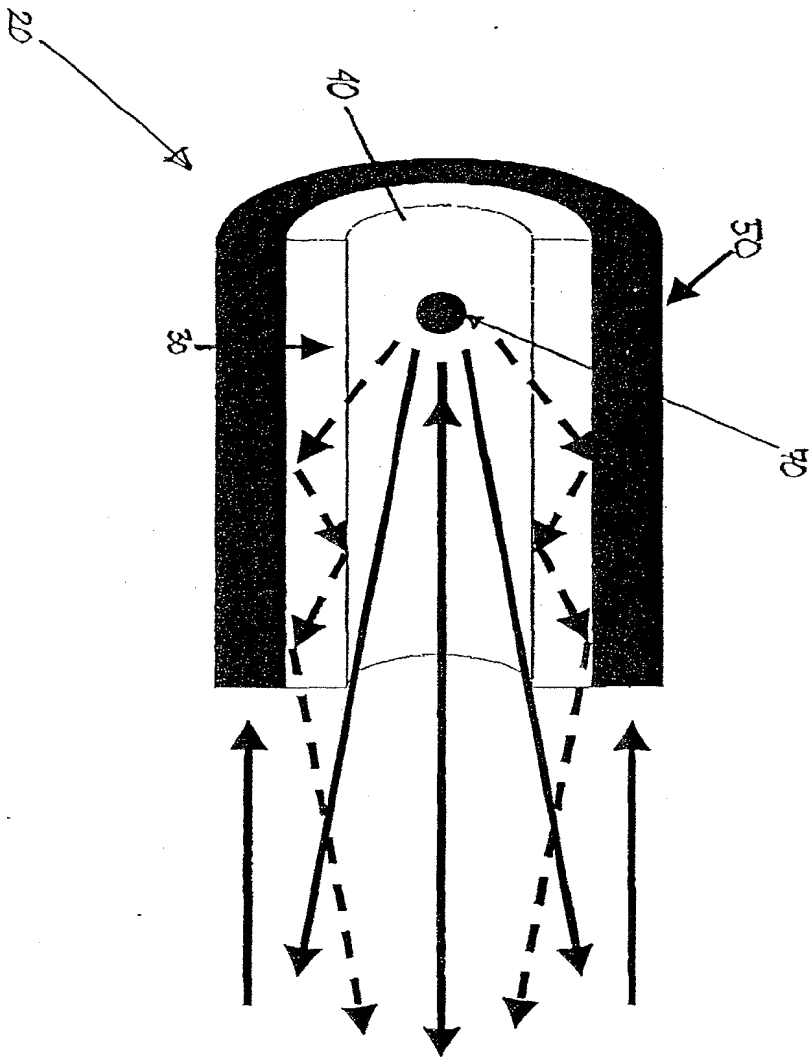


FIG. 3

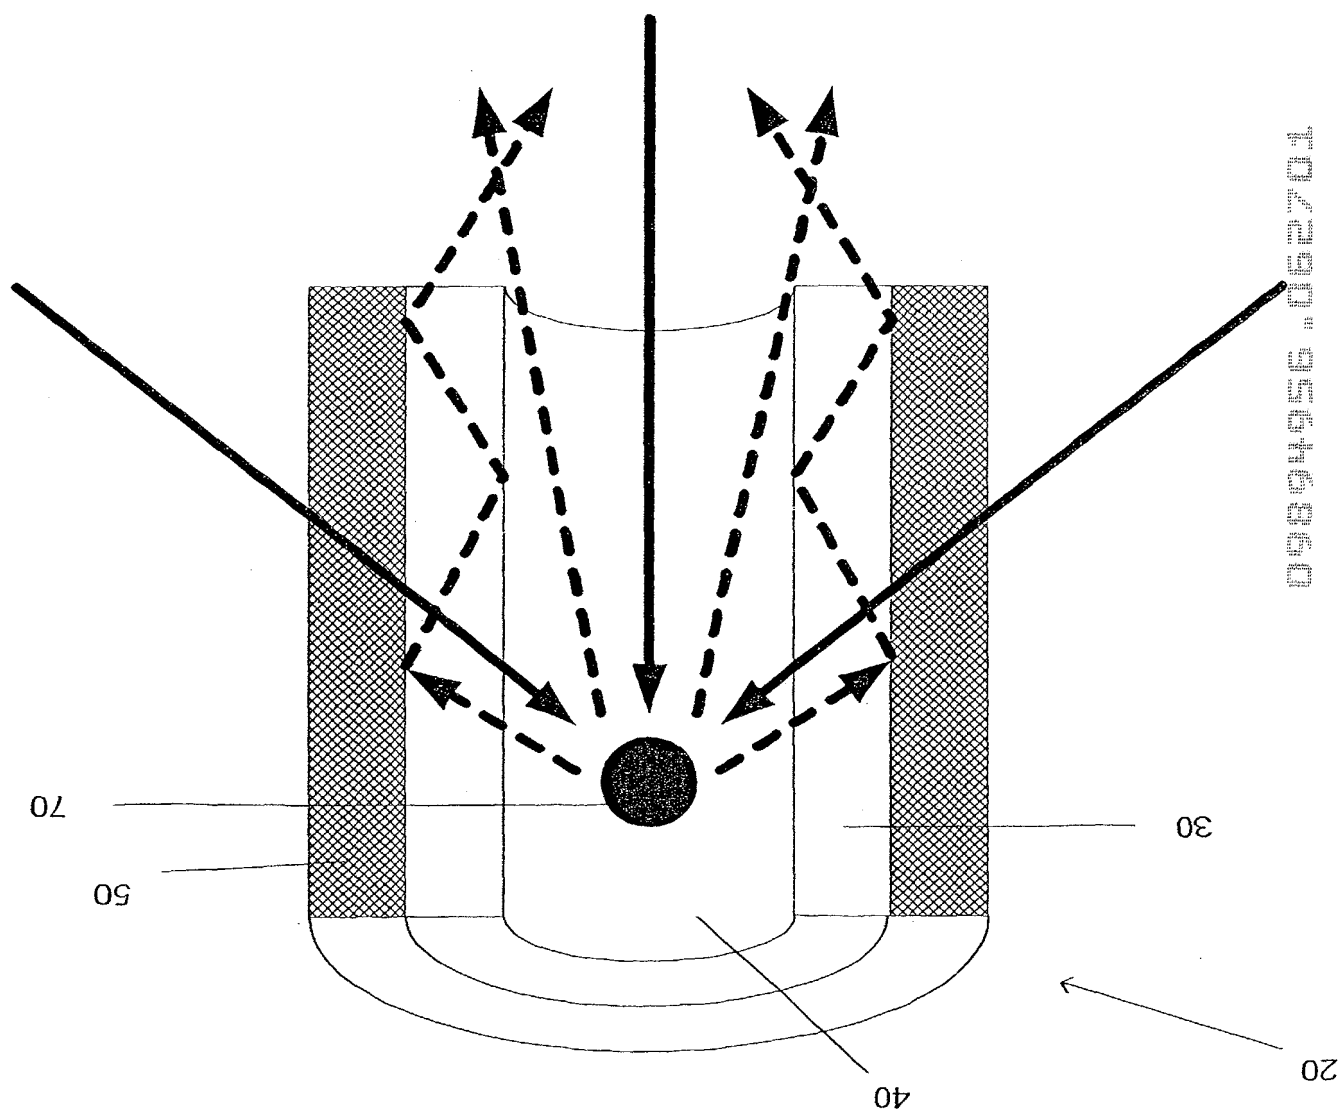


FIG. 4

102290 95646860

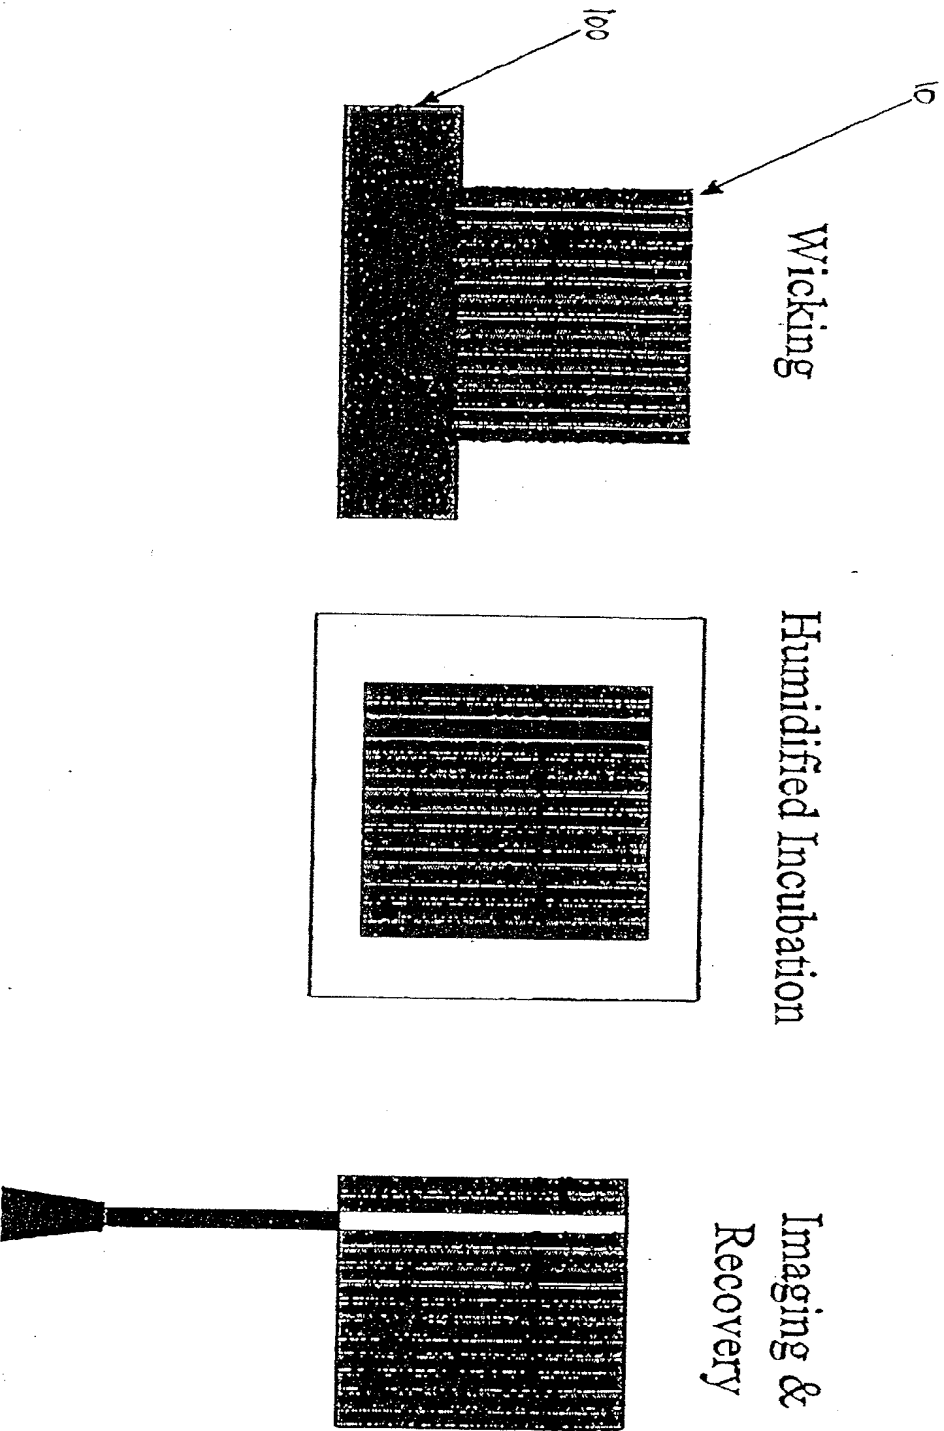


FIG. 5

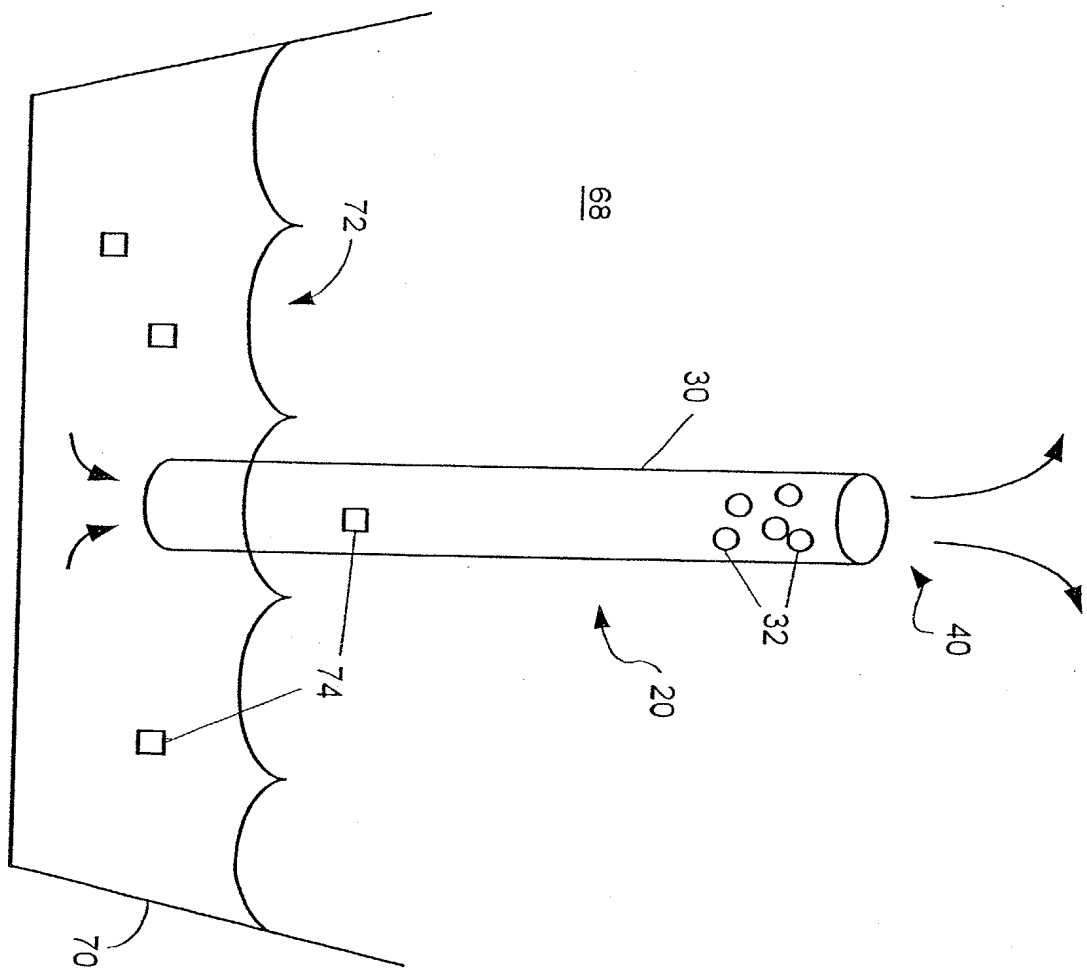


FIG. 6

10,2290 95646860

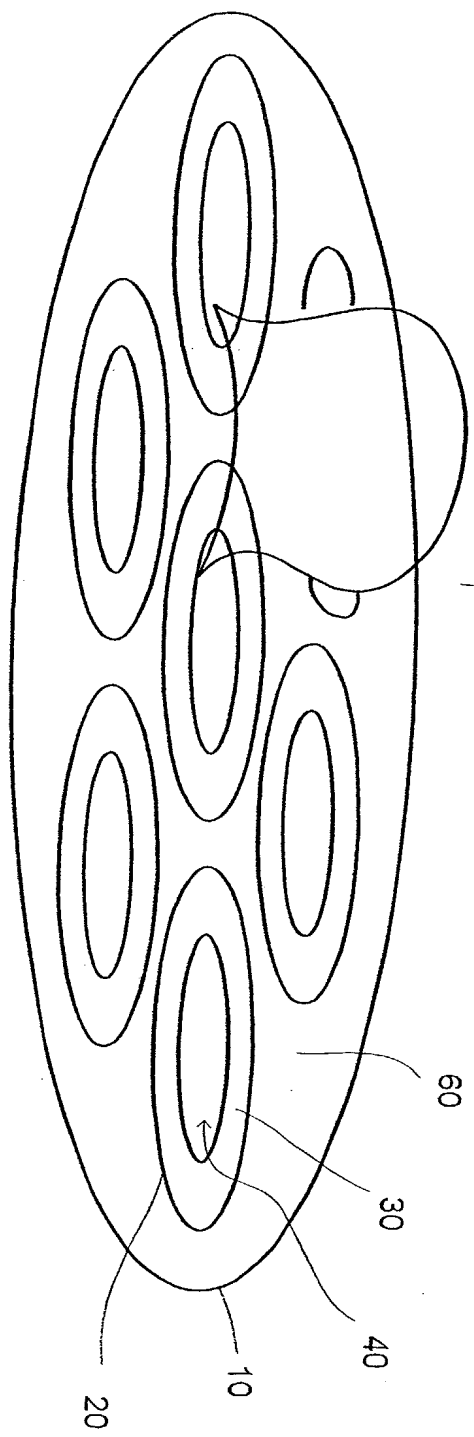


FIG. 7A



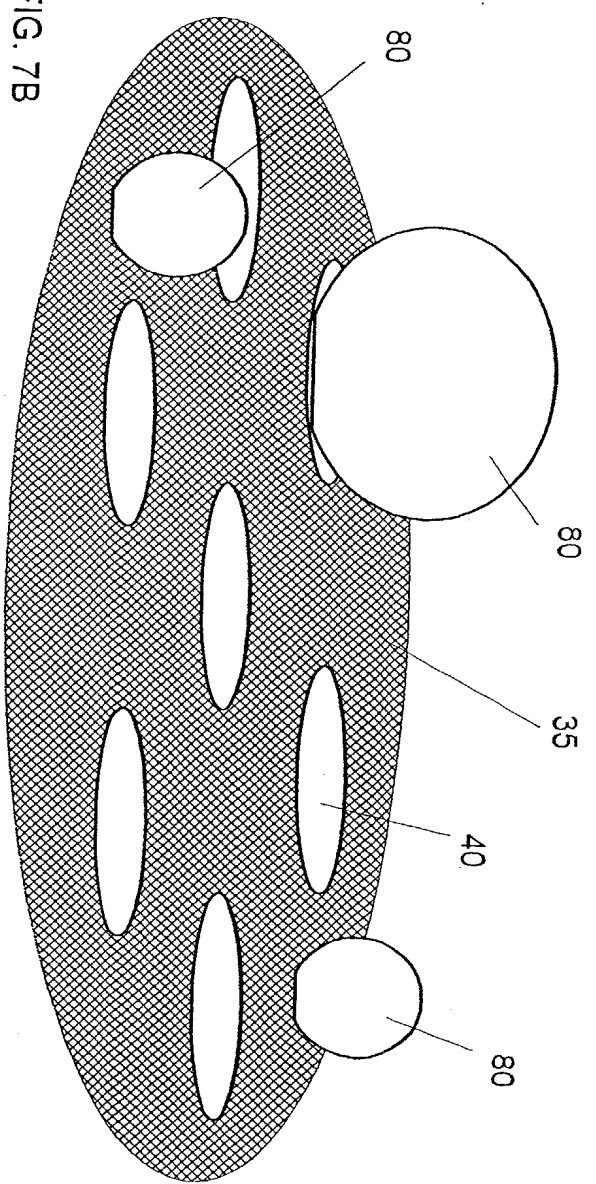



FIG. 7B

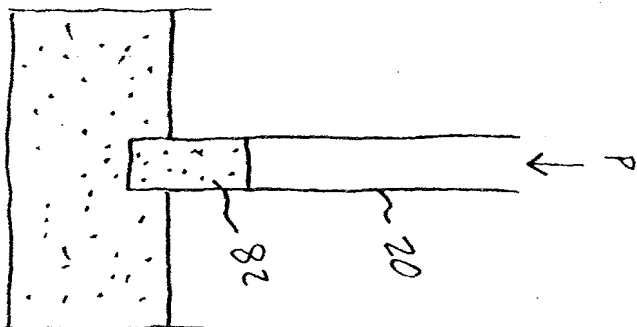

A.

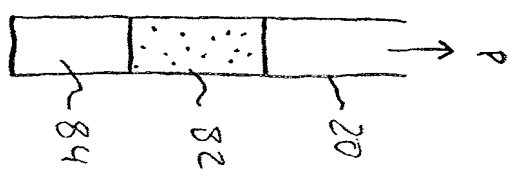

B.

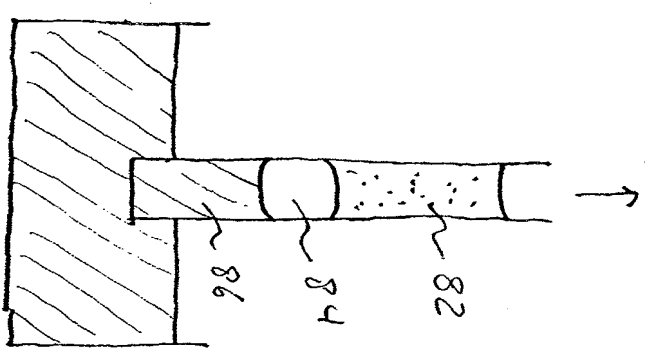

C.

FIG. 8

1042290" 95646880

Capillary array.

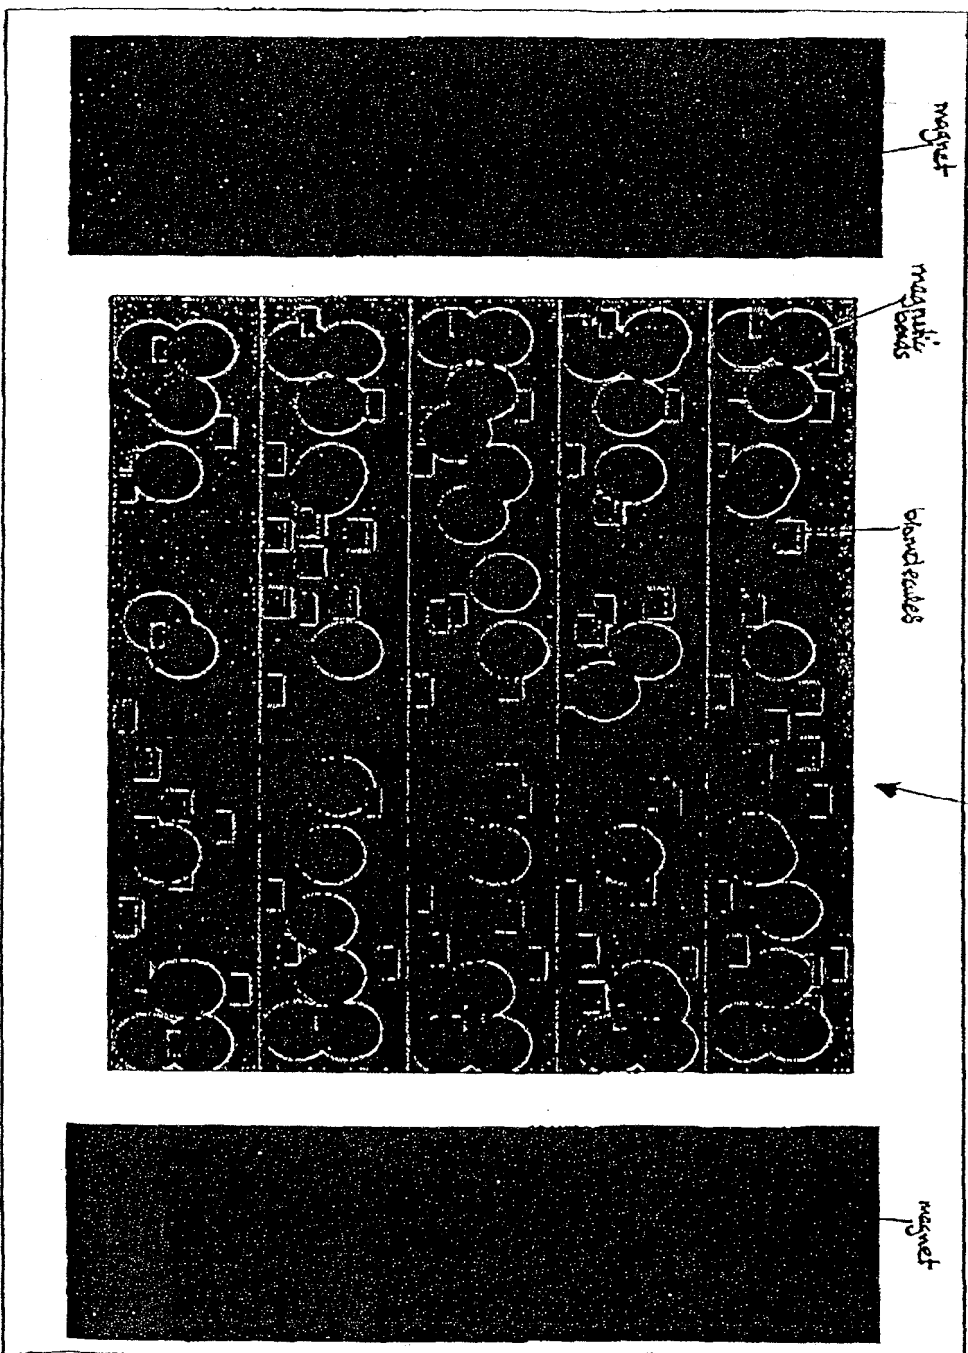


FIG. 9A

102290 95646860

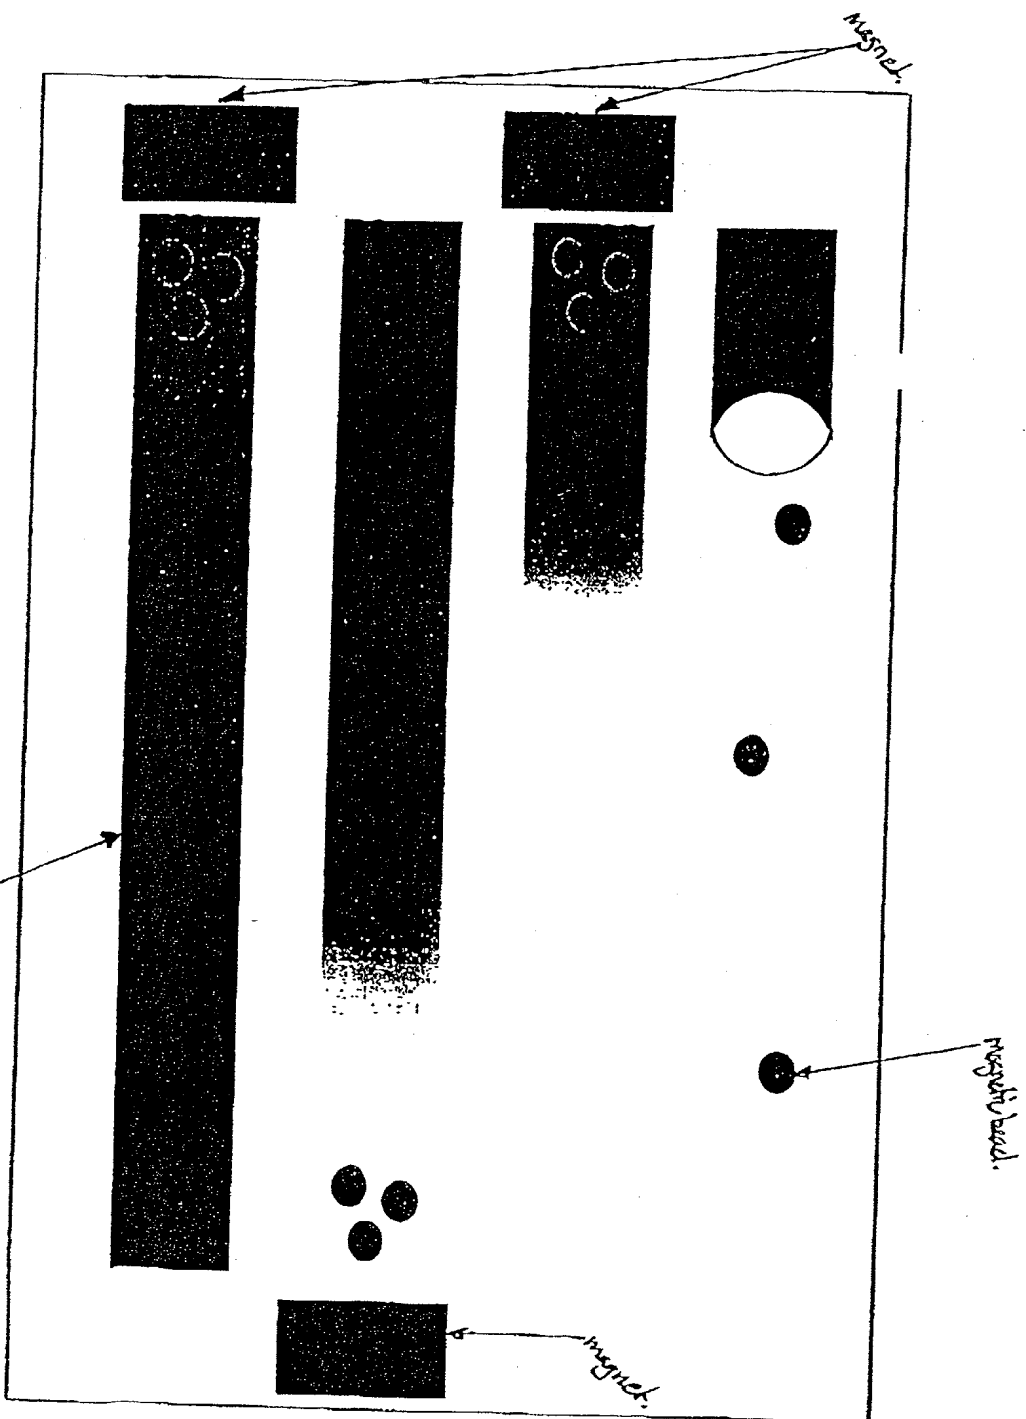


FIG. 9B

09894956 062701


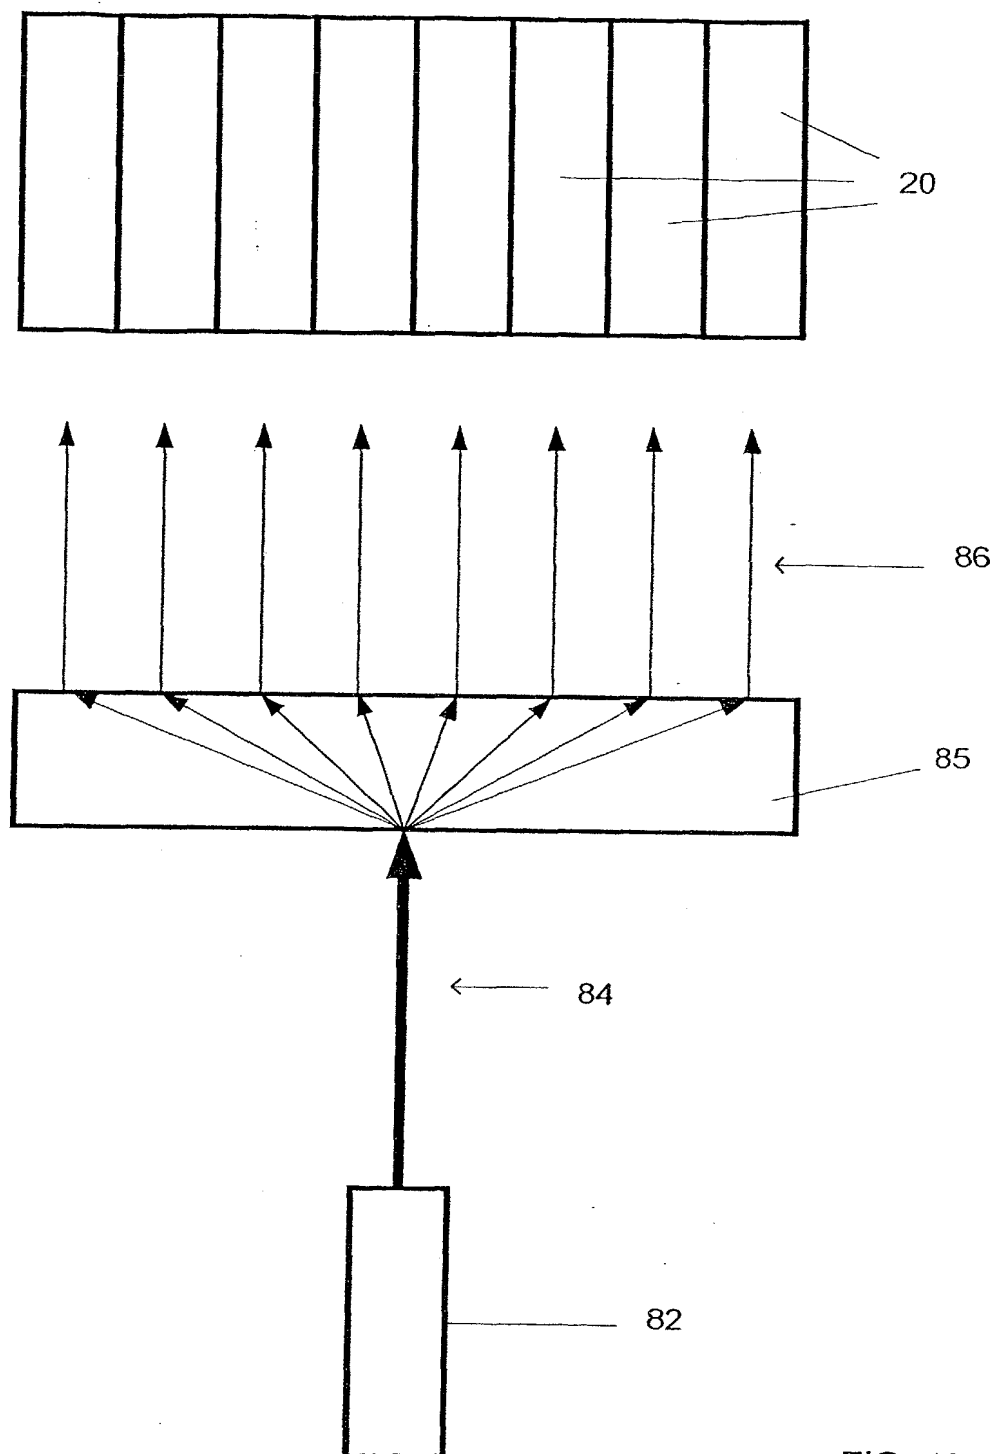


FIG. 10


Automated Hit Detection & Recovery System

FIG. 11


100

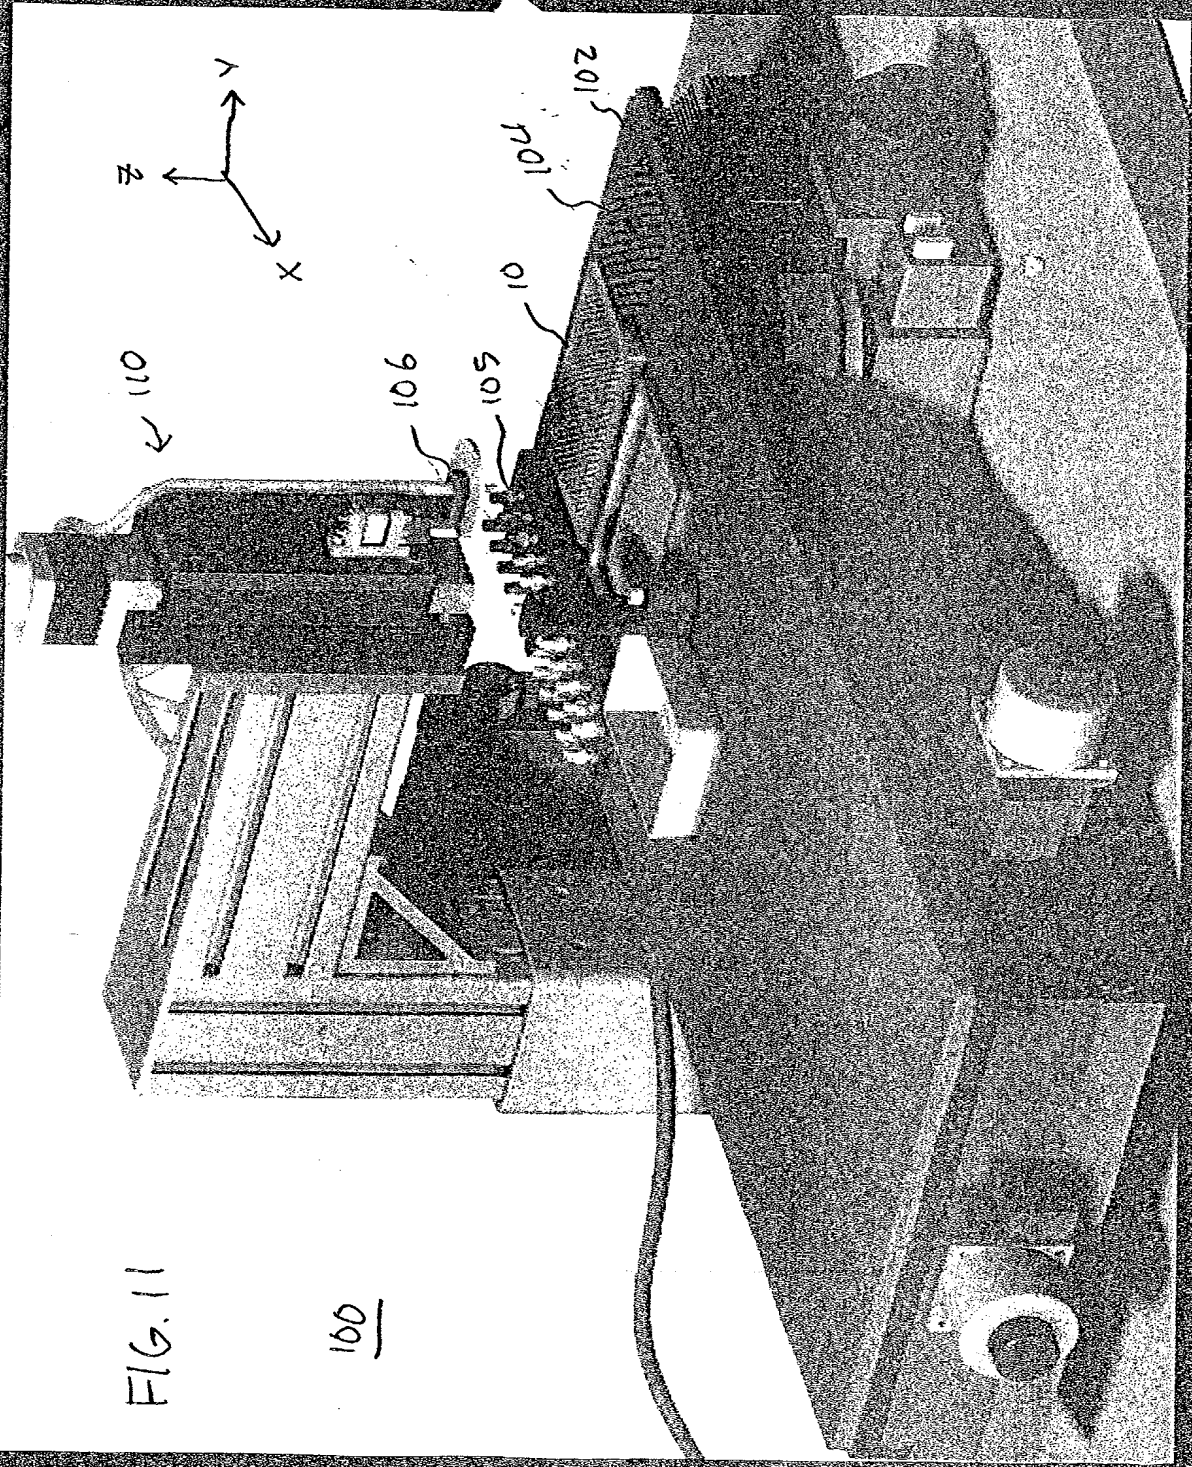

0594956 .062701

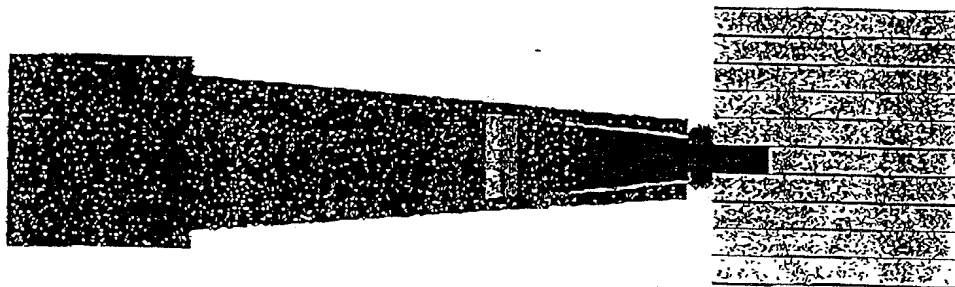

A

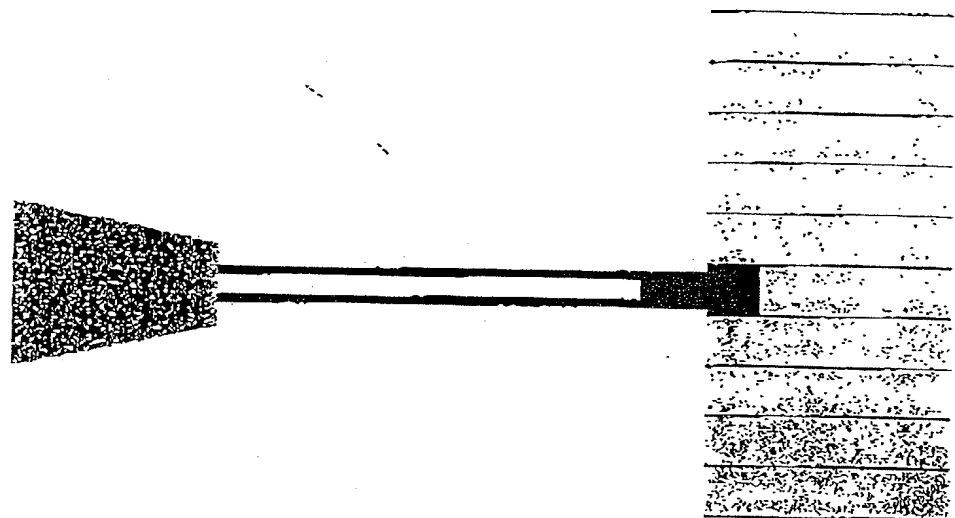

B

FIG. 12

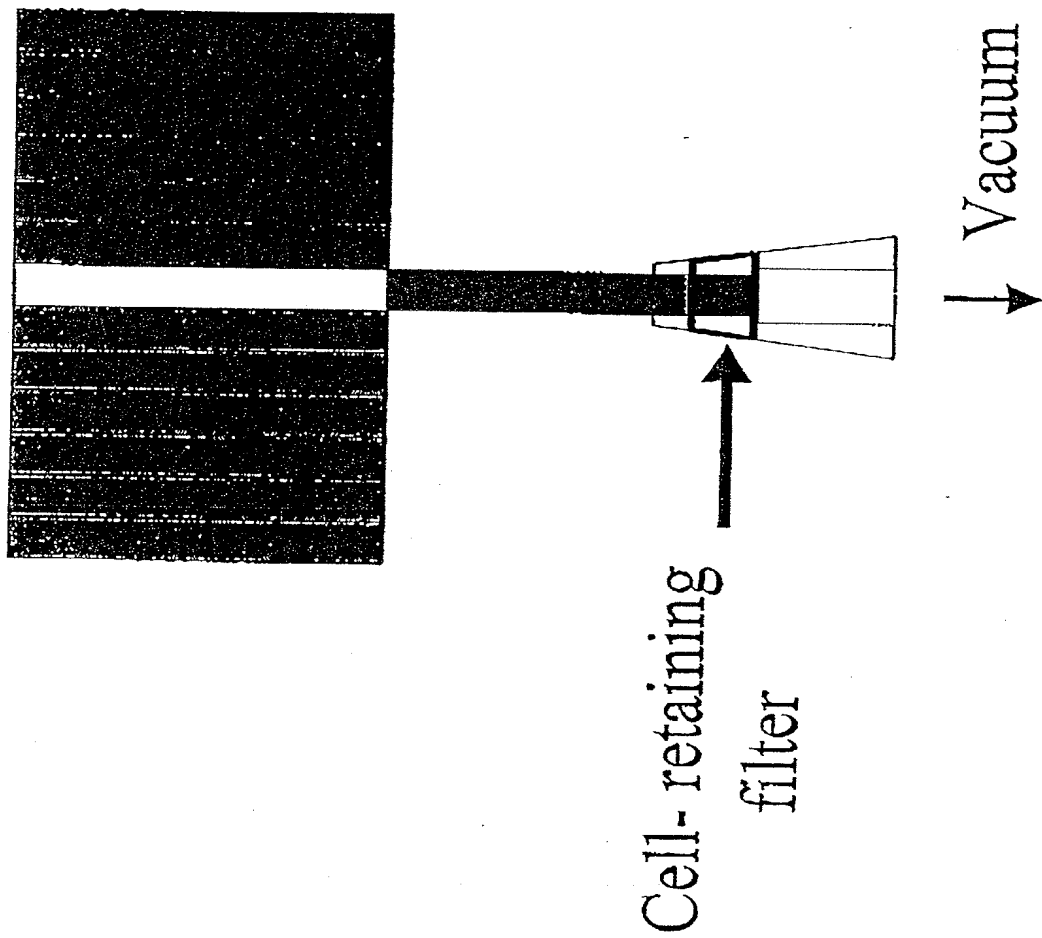


FIG. 12C

TO/290" 95546860

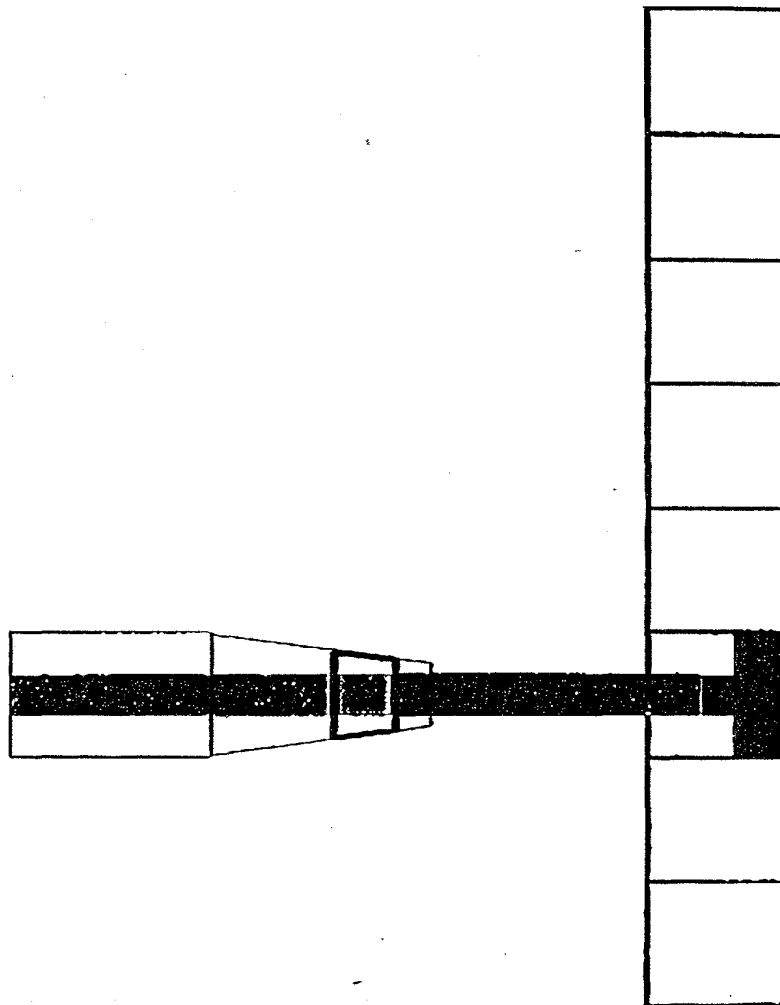


FIG. 12 D